


Emergency Department

**LIFEPAK 20**  
DEFIBRILLATOR/MONITOR

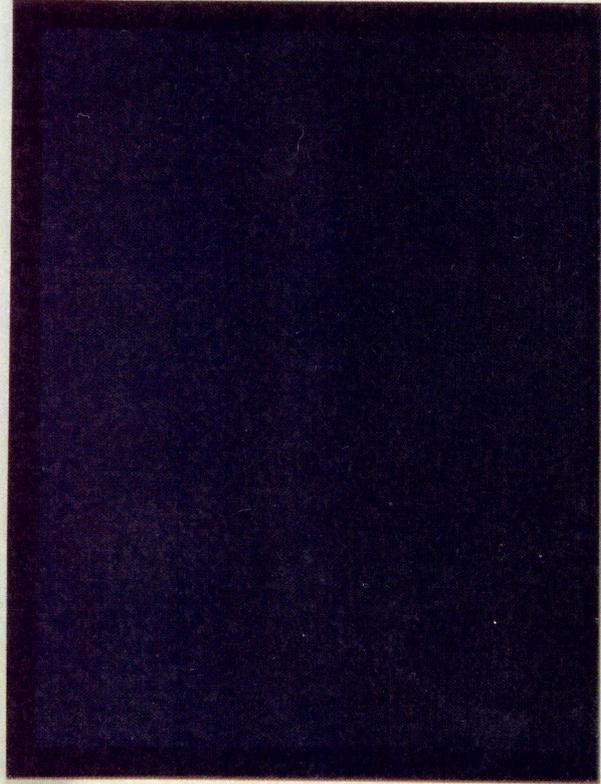

1 ON

2 ENERGY SELECT

3 CHARGE

⚡

AED MODE

ANALYZE

LEAD

SIZE

SYNC

PACER

RATE

CURRENT

PAUSE

ALARMS

OPTIONS

EVENT

Speed Dial

PRINT

CODE SUMMARY

AC Mains

Service



ECG



For use only by qualified personnel.  
All uses in the presence of flammable gases.



Emergency Department

**LIFEPAK 20**  
DEFIBRILLATOR/MONITOR



1 ON

2 ENERGY SELECT

3 CHARGE

ANALYZE

AED MODE

LEAD SIZE SYNC

PACER RATE CURRENT PAUSE

ALARMS OPTIONS

PRINT CODE SUMMARY

AC Mains Service

EVENT Speed Dial

Medtronic

ECG



Read. For use only by qualified personnel. For use in the presence of flammable gases.

201897

Emergency Department

**LIFEPAK 20**  
DEFIBRILLATOR / MONITOR

HR **224**

II X3



5J Selected  
8:36:31



Paddles

Check Printer

PRINT

CODE  
SUMMARY

AC Mains

Service



**Medtronic**

ECG



Book for use only by qualified personnel.  
Not use in the presence of flammable gases.

1 ON

2 ENERGY  
SELECT

3 CHARGE



AED MODE

ANALYZE

LEAD

SIZE

SYNC

PACER

RATE

CURRENT

PAUSE

ALARMS

OPTIONS

EVENT


Speed Dial



507897

Emergency Department

**LIFEPAK 20**  
DEFIBRILLATOR/MONITOR

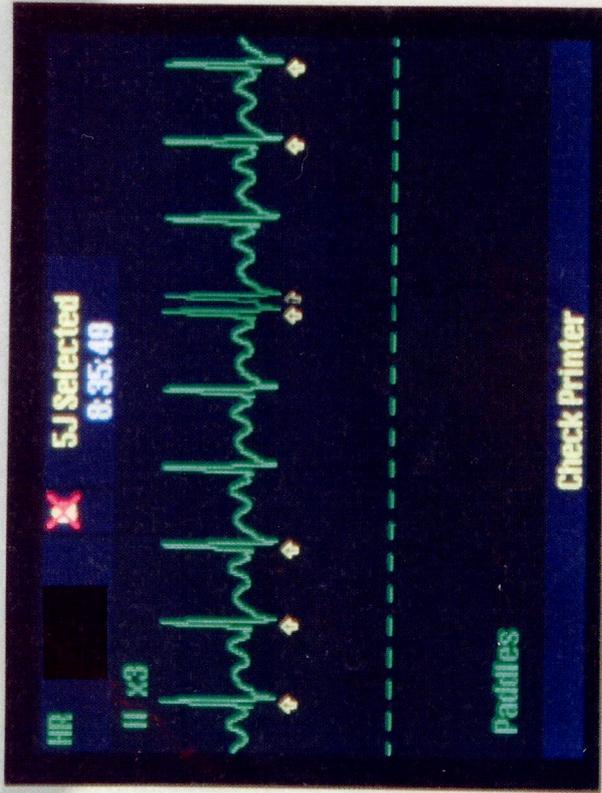

1 ON  
2 ENERGY SELECT  
3 CHARGE

AED MODE ANALYZE

LEAD SIZE SYNC

PACER RATE CURRENT PAUSE

ALARMS OPTIONS

PRINT CODE SUMMARY AC Mains Service

EVENT Speed Dial

**Medtronic**

EGG-101



Read the manual for use with qualified personnel. Do not use in the presence of flammable gases.